


Software Version : 6.3.0.0445
 Sample Name : malaixianyaan
 Instrument Name : PELC
 Rack/Vial : 0/1
 Sample Amount : 1.000000
 Cycle : 1

Date : 11/6/2009 4:23:01 PM
 Data Acquisition Time : 11/6/2009 4:05:11 PM
 Channel : A
 Operator : manager
 Dilution Factor : 1.000000

Result File :

Sequence File : C:\PenExe\TcWS\Ver6.3.0\Examples\--20091106-155115.seq

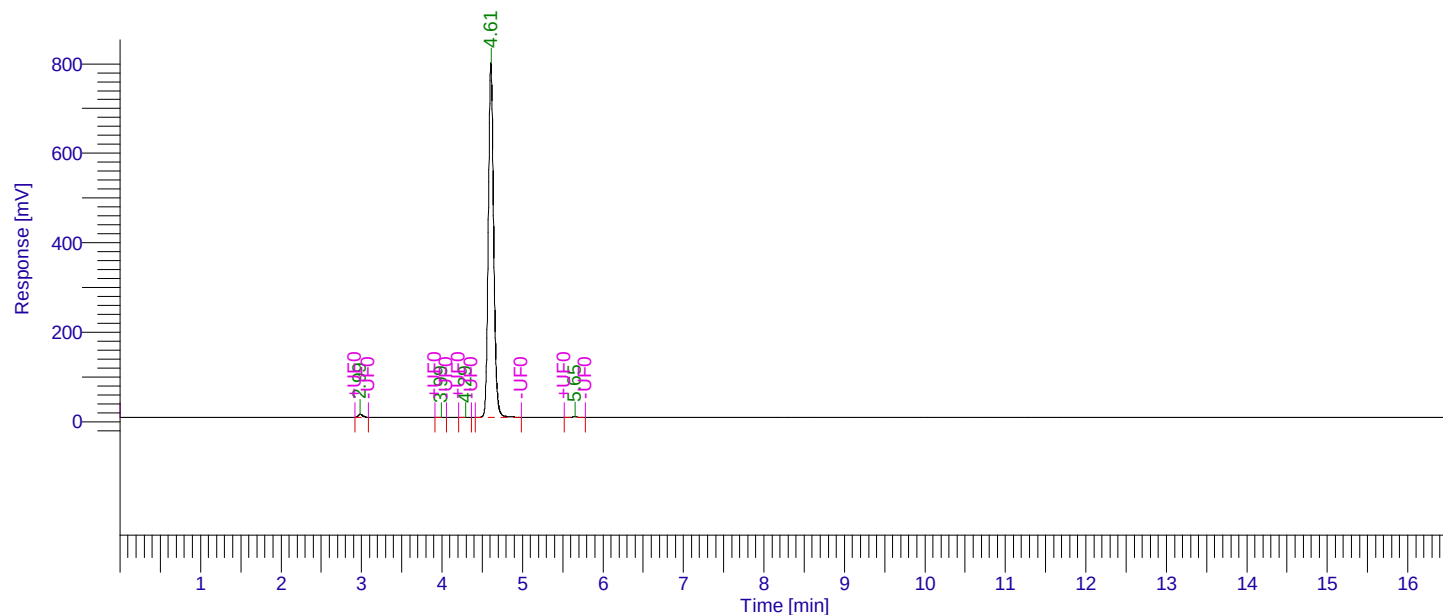

Test REPORT

Peak #	Component Name	Time [min]	Area [uV*sec]	Height [uV]	Area [%]	Norm. Area [%]	BL
1		2.985	23721.21	6659.23	0.64	0.64	MM
2		3.990	817.06	225.77	0.02	0.02	MM
3		4.292	823.08	201.11	0.02	0.02	MM
4		4.608	3650280.75	792218.07	99.18	99.18	MM
5		5.650	4752.93	877.74	0.13	0.13	MM
			3680395.03	800181.91	100.00	100.00	

Missing Component Report

Component Expected Retention (Calibration File)

All components were found