

File D:\DATA\T91\MONITOR\CP-0006590-101-00019-LCMSA033.D

Injection Date : 25 Feb 12 10:39 am +0800

Tgt Mass (EZX) : 179.00

Sample Name : CP-0006590-101

Location : P1-A-05

Acq. Operator : T91-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : D:\METHODS\1-POS-MON-3MIN.M

Analysis Method : D:\METHODS\1-POS-MON-3MIN.M

Sample Info : 179.00

Method Info : Column: SunFire C18, 4.6x50mm, 3.5um


Mobile phase: H2O(0.05%TFA) (A) / ACN(0.05%TFA) (B)

Elution program: Gradient from 5 to 95% of B in 1.2min at 2ml/min


Temperature: 50 °C

Detection: UV (214 , 4 nm) and MS (ESI, Pos mode ,70 to 1000 amu)


*ADC1 A, ELSD

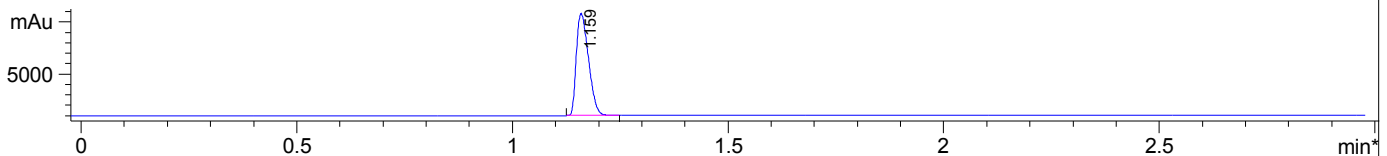


*DAD1 A, Sig=214,4 Ref=off

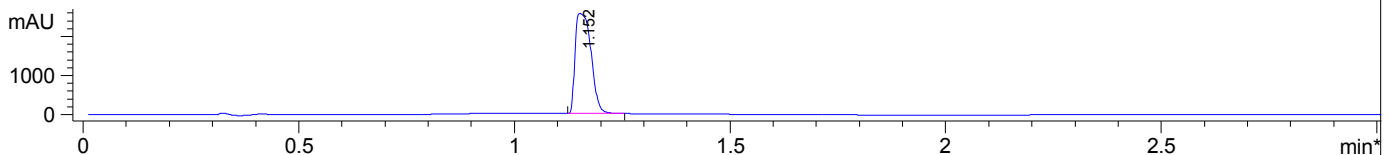


*DAD1 B, Sig=254,4 Ref=off

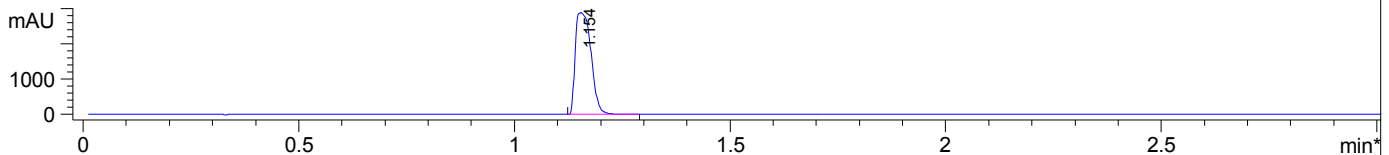

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

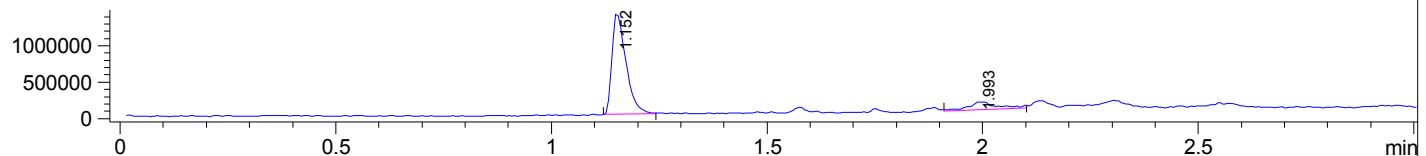

Ion 180, MSD1 180, Target Mass 179 +H Positive, EIC=179.7:180.7

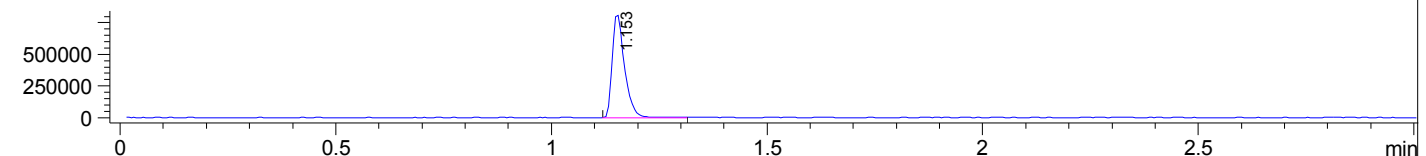

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.16	0.03	19273.67	9791.97	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.15	0.04	6537.47	2557.93	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.15	0.04	7304.19	2886.78	100.00

Ret. Time: 1.15

<<<< POSITIVE SPECTRA >>>>

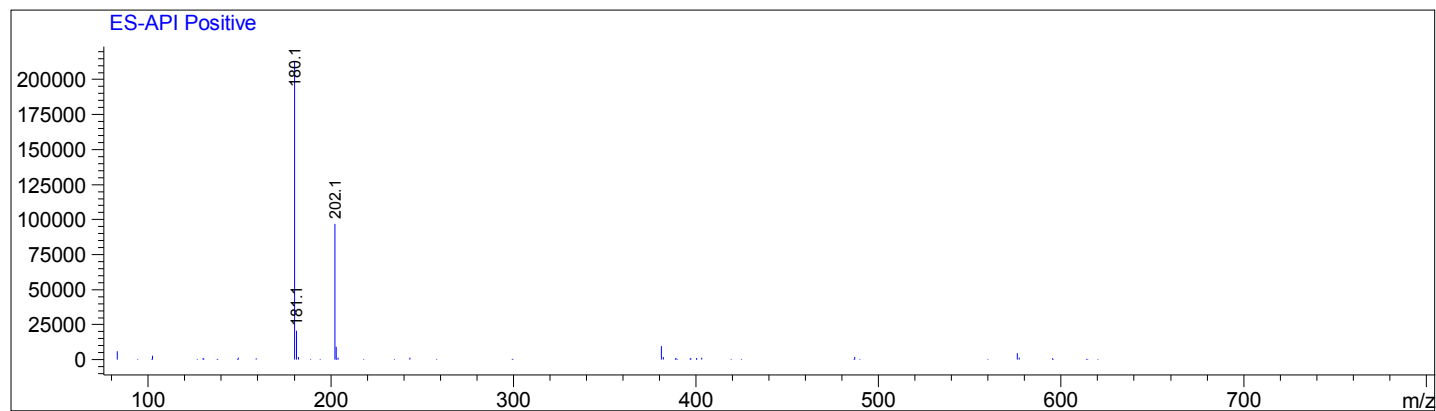

Ret. Time: 1.99

