

File D:\DATA\PREP\MONITOR\253-1-03220-LCMSA023.D

Injection Date : 1 Mar 12 5:36 pm +0800

Tgt Mass (EZX) : 253.00

Sample Name : 253-1

Location : P1-A-02

Acq. Operator : PREP

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 3 ul

Acq. Method : D:\METHODS\2-NEG-MON-1.M

Analysis Method : D:\METHODS\2-NEG-MON-1.M

Sample Info : 253.00

Method Info : Column:Xbrige C18 (4.6x 50 mm,3.5um)


Mobile phase: H2O(10 mmol NH4HCO3) (A) / ACN(B)

Elution program: Gradient from 10 to 95% of B in 1.5min at 1.8ml/min


Temperature: 50 °C

Detection: UV (214 , 4 nm) and MS (ESI, Neg mode ,80 to 1000 amu)


*DAD1 A, Sig=214,4 Ref=off

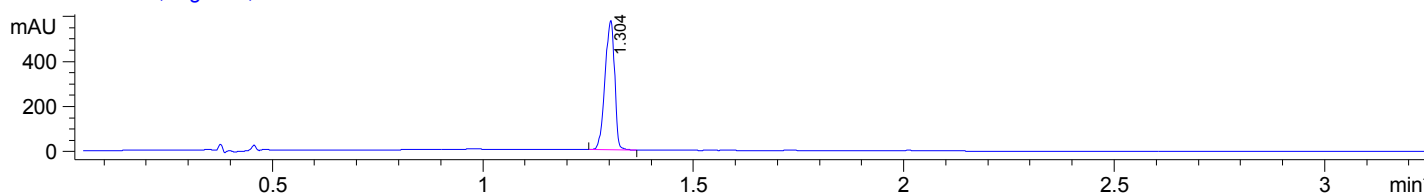


*DAD1 B, Sig=254,4 Ref=off

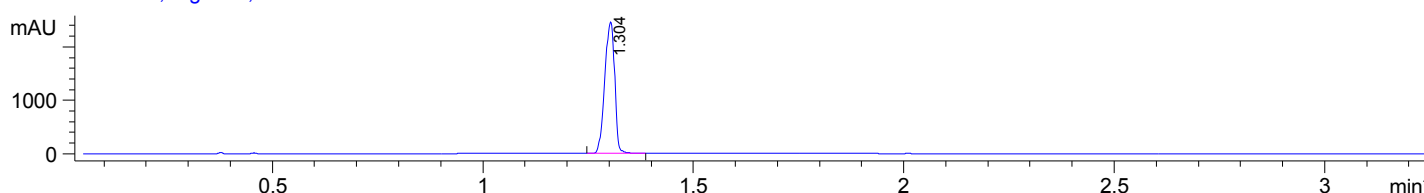

MSD1 TIC, MS File ES-API, Neg, Scan, Frag: 80

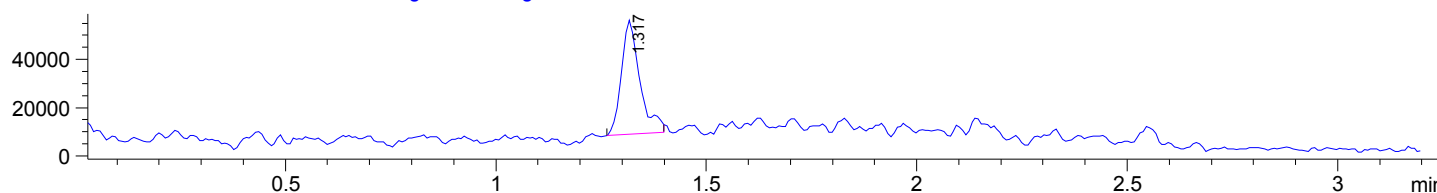

Ion 252, MSD1 252, Target Mass 253 -H Negative, EIC=251.7:252.7

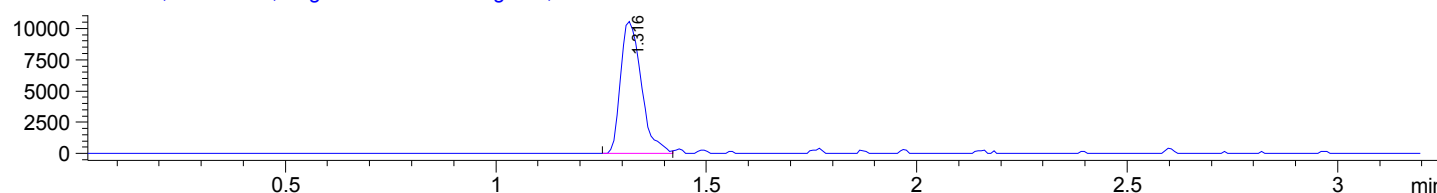

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.30	0.03	913.12	574.52	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.30	0.03	4031.51	2464.39	100.00

Ret. Time: 1.32

<<<< NEGATIVE SPECTRA >>>>

